



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100422

Report Issue Date: 05/07/2025
Date Received: 2024-07-26
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.079	AG335202	0.079	0.079	0.079	0.079	0.079	0.079	0.079
0.300	0.297	AG327804	0.293	0.293	0.294	0.294	0.293	0.293	0.293

As Found - Evaluation Analyst: Colleen O'Bryant
 As Found Conditions - Barometric Pressure (inHg): 29.88 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.1 Relative Humidity (%): 56
 As-Found Lab Activity Date Range: 07/26/2024 - 07/29/2024

Screen experienced intermittent response issues during as-found linearity. Recommend repair to troubleshoot.

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG408002	0.020	0.020	0.020	0.021	0.020	0.020	+/- 0.002	
0.040	0.039	AG407908	0.039	0.040	0.040	0.040	0.039	0.040	+/- 0.003	
0.080	0.079	AG335202	0.078	0.078	0.078	0.079	0.079	0.078	+/- 0.004	
0.100	0.098	AG333401	0.100	0.099	0.099	0.099	0.100	0.099	+/- 0.004	
0.150	0.148	AG332004	0.147	0.146	0.146	0.145	0.146	0.146	+/- 0.006	
0.300	0.295	AG427706	0.295	0.294	0.295	0.296	0.295	0.295	+/- 0.012	

As Left Conditions - Barometric Pressure (inHg): 29.44 Barometer Used: VWR S/N 240680771 Temperature (C): 23.4 Relative Humidity (%): 23
 As-Left Lab Activity Date Range: 04/29/2025 - 04/29/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 04/29/2025

kaija.swisher@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 05/07/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100422 Analyst or Technician Name: Kaija Swisher
DataMaster DMT Calibration Start Date: 4/29/25

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 290680771
Calibration Due Date: 9/10/26
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.49 Temperature(C) 23.4 Relative Humidity(%) 23
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) – *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250219KS Expiration Date: 5/19/25
Simulator S/N: SD1200 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 2050219KS Expiration Date: 5/19/25
Simulator S/N: SD1198 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 232P41233 Expiration Date: 5/19/25
Simulator S/N: SD1199 Thermometer Verification Performed? 9/20/25 (solution)

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/25

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 4/29/25
Data Interpretation Date (Technician): _____ (if applicable)
Data Interpretation Date (Analyst): 4/29/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 08:30:36

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 2.04 V PASSED
(1.22 V - 2.86 V)
Cooler Voltage = 1.80 V PASSED
(1.08 V - 2.52 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 528 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.4 in

PUMP INFO

Flow Rate = 4.941 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED
Xq = 0.110 0.24% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 8:42 AM

Temperatures (°C)
Sample Cell: 48.9°C
Breath Tube: 47.2°C

Current Barometer 29.4 in
Volume (Ltr) 1.55

Settings
Lamp: 2.04 V
Bias: 80 V
Cooler: 1.80 V
Chopper: 526 Hz

Voltages (V)
Flow: 1.06 V
Detector: 0.027 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/22/2025
Time: 11:09:21

OPERATOR NAME:
MEGAN CARLOCK
CERTIFICATE #: 10747

Ca = 0.1000
CAL = 1.003444 0.800 <= CAL < 1.200
b1 = 0.0006 0.0000 <= b1 < 0.0040
b2 = 0.0067 0.0010 <= b2 < 0.0100
b3 = 0.0010 0.0000 <= b3 < 0.0040
Xq = 0.1095 0.0500 <= Xq < 0.2000
a21 = 1.215930 1.050 <= a21 < 1.300
a31 = 0.412580 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 08:44:49


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:45
BLANK TEST	0.000	08:46
INTERNAL STANDARD	VERIFIED	08:46
EXTERNAL STANDARD	0.078	08:46
BLANK TEST	0.000	08:47
SUBJECT SAMPLE (Vol=1.58L)	0.000	08:48
BLANK TEST	0.000	08:49
EXTERNAL STANDARD	0.079	08:49
BLANK TEST	0.000	08:50

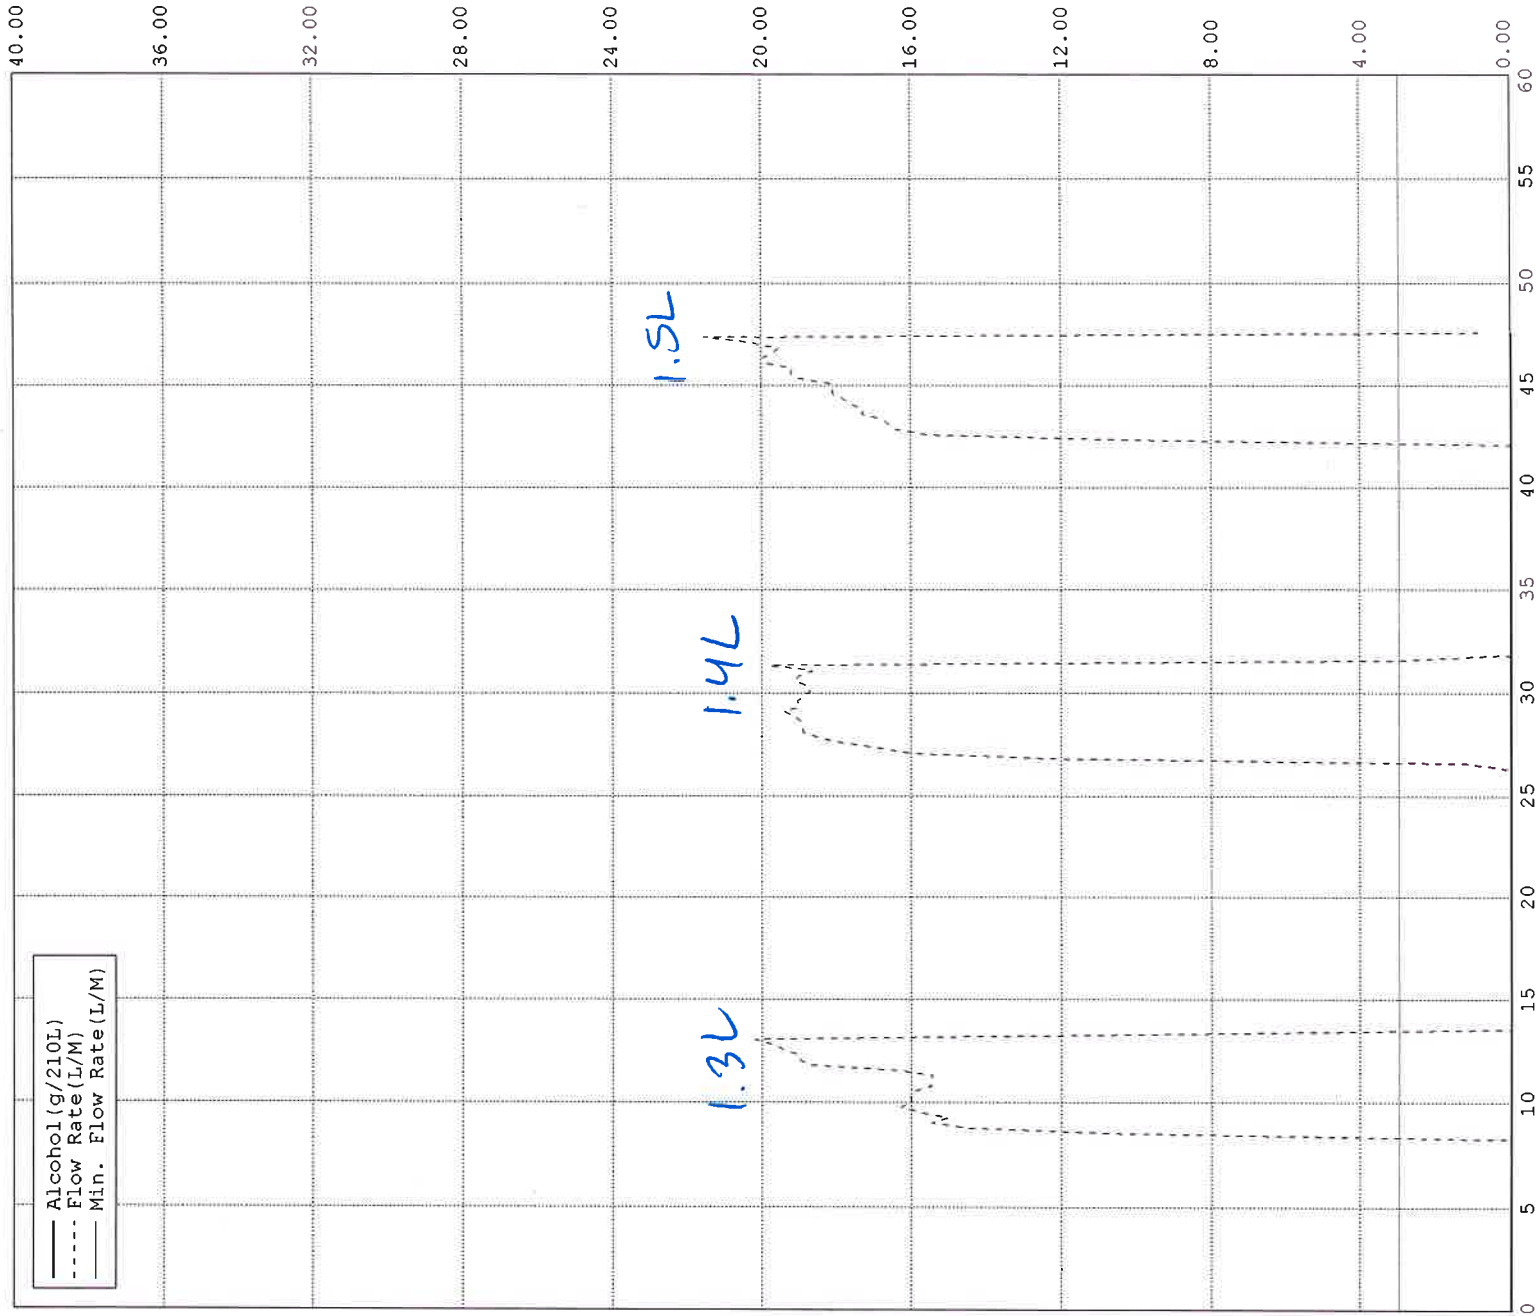

KS

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100422

Date: 04/29/2025
 Time: 08:54:48

SUPERVISOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.039	0.0396	0.0005
0.079	0.0784	0.0005
0.098	0.0994	0.0005
0.148	0.1460	0.0007
0.295	0.2950	0.0007

SLOPE = 0.997322
 R² = 0.999872

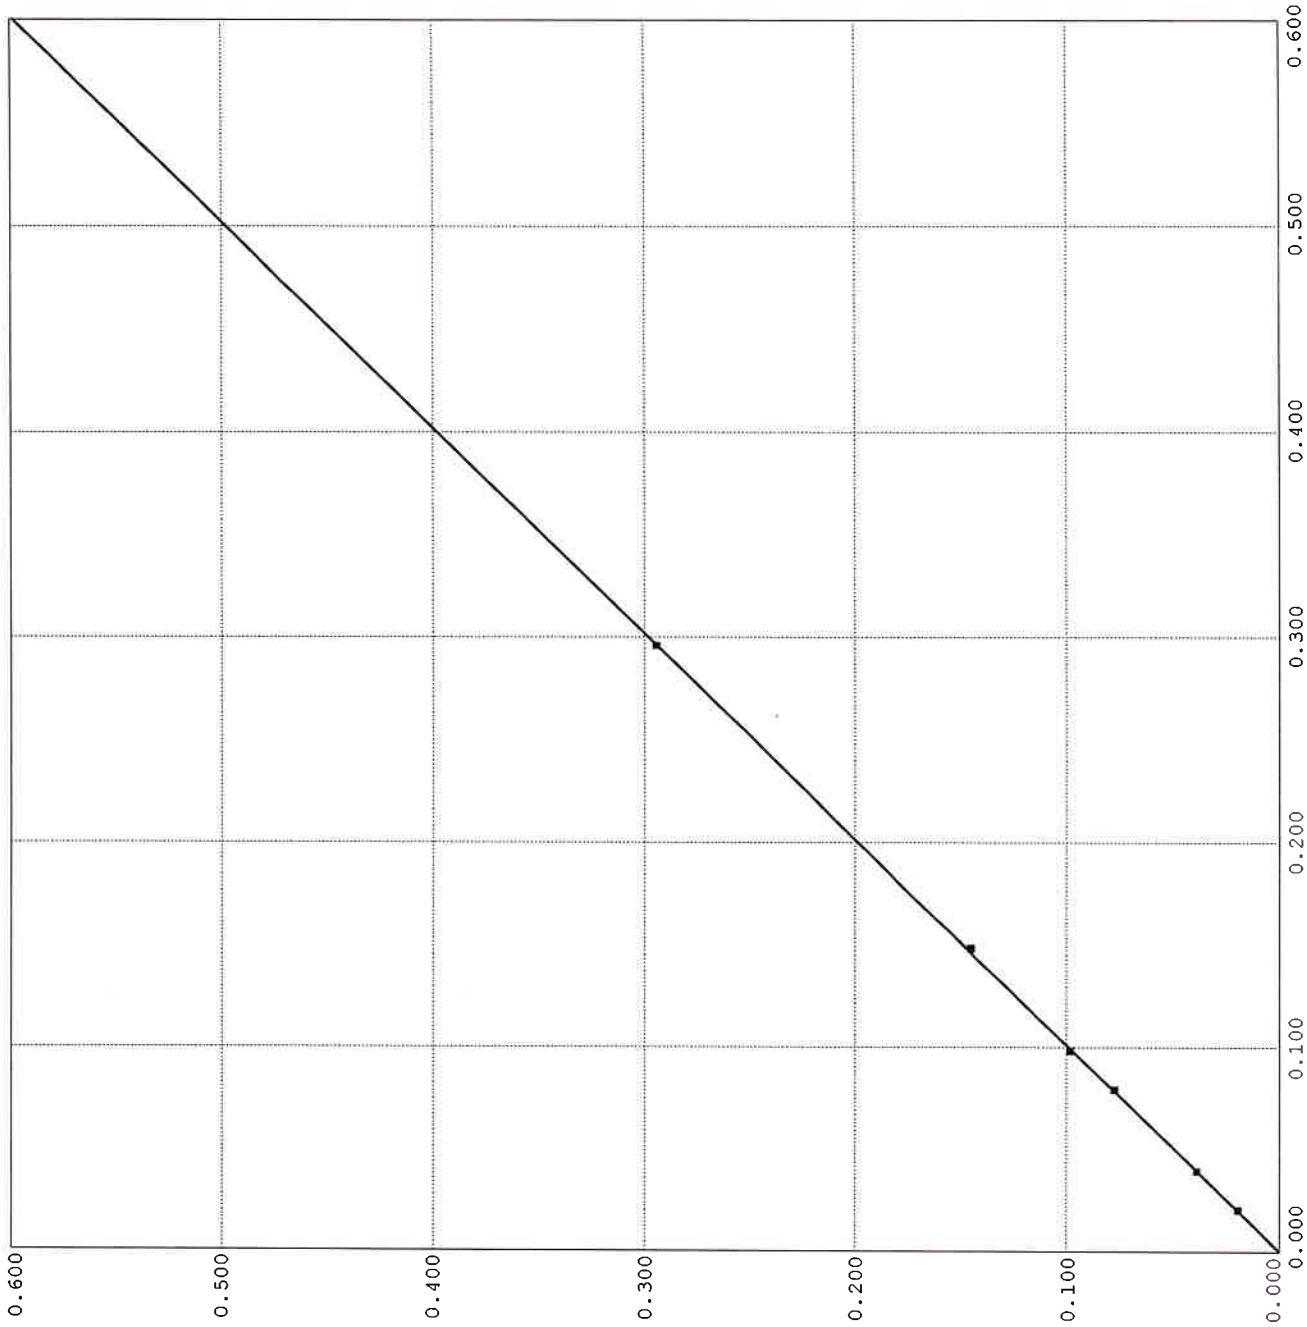

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100422






Date: 04/29/2025
Time: 08:54:51

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.44: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 1023 psi

BLANK TEST	0.000	08:56
INTERNAL STANDARD	VERIFIED	08:56
EXTERNAL STANDARD	0.020	08:56
BLANK TEST	0.000	08:57
EXTERNAL STANDARD	0.020	08:57
BLANK TEST	0.000	08:58
EXTERNAL STANDARD	0.020	08:58
BLANK TEST	0.000	08:59
EXTERNAL STANDARD	0.021	08:59
BLANK TEST	0.000	09:00
EXTERNAL STANDARD	0.020	09:01
BLANK TEST	0.000	09:01

Average = 0.0202
Std Dev = 0.0004

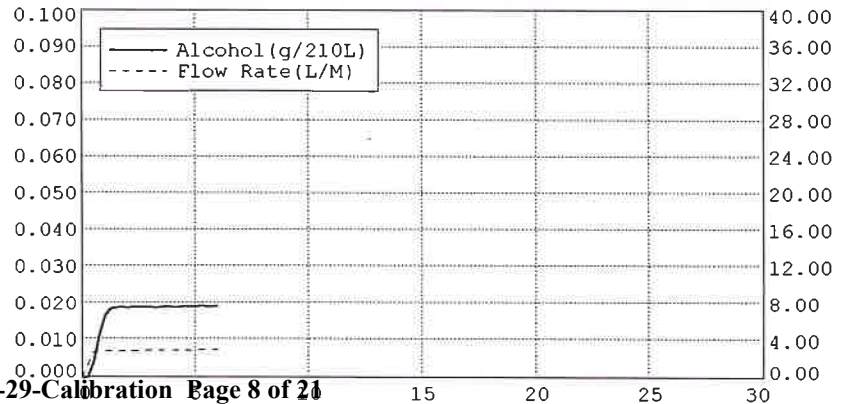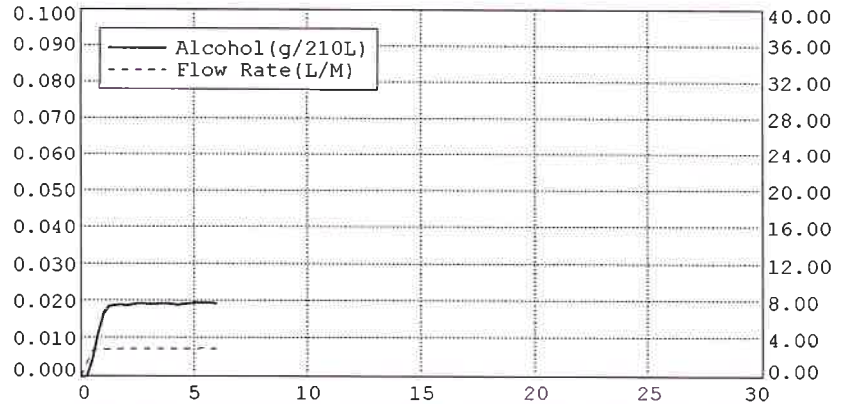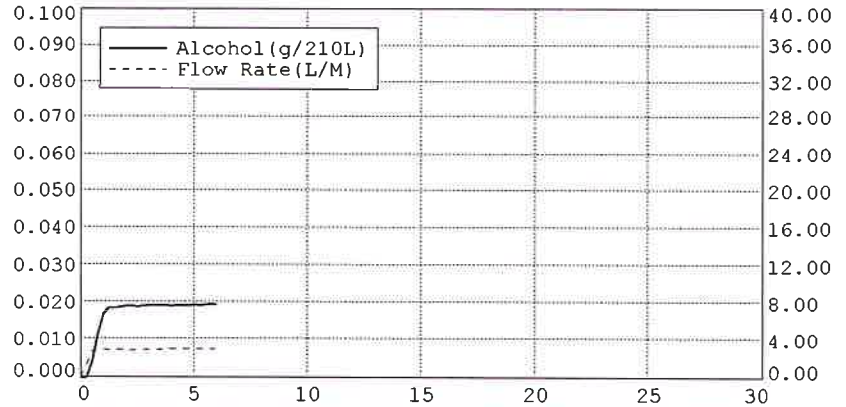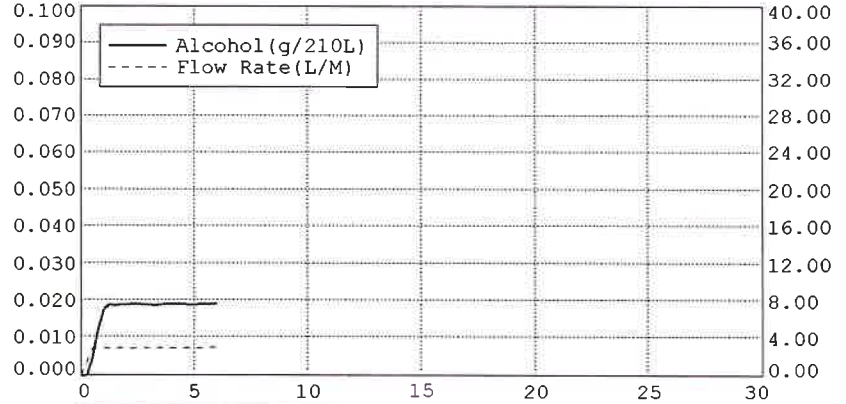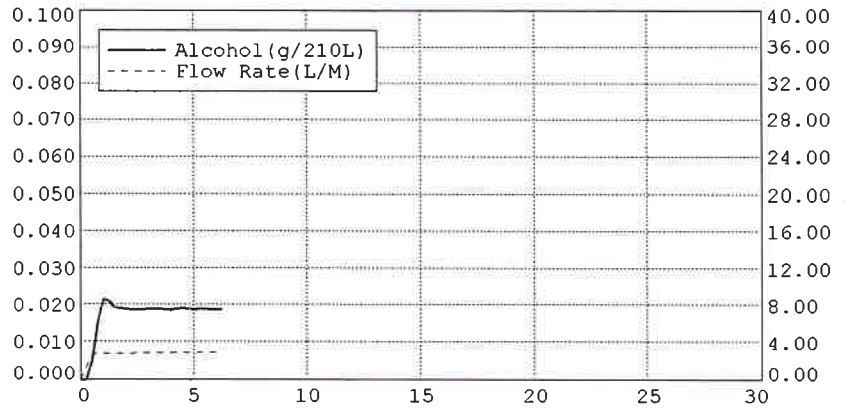

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100422






Date: 04/29/2025
 Time: 09:02:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.45: 0.039
 LOT #: AG407908
 EXPIRATION: 03/19/2026
 TANK PRESSURE: 917 psi

BLANK TEST	0.000	09:04
INTERNAL STANDARD	VERIFIED	09:04
EXTERNAL STANDARD	0.039	09:04
BLANK TEST	0.000	09:05
EXTERNAL STANDARD	0.040	09:05
BLANK TEST	0.000	09:06
EXTERNAL STANDARD	0.040	09:06
BLANK TEST	0.000	09:07
EXTERNAL STANDARD	0.040	09:08
BLANK TEST	0.000	09:08
EXTERNAL STANDARD	0.039	09:09
BLANK TEST	0.000	09:10

Average = 0.0396
 Std Dev = 0.0005

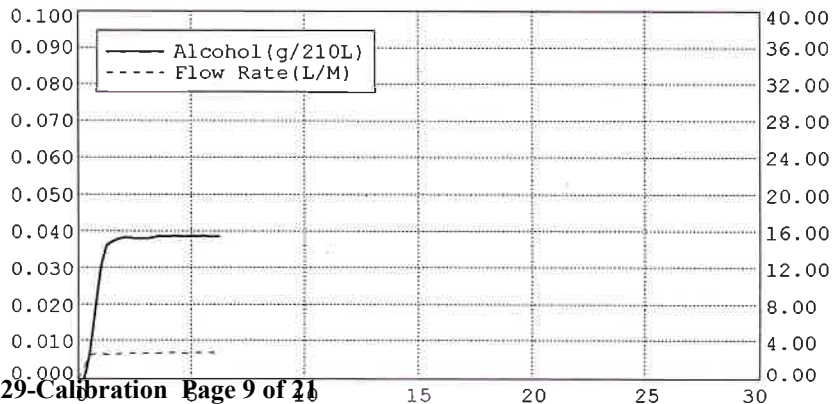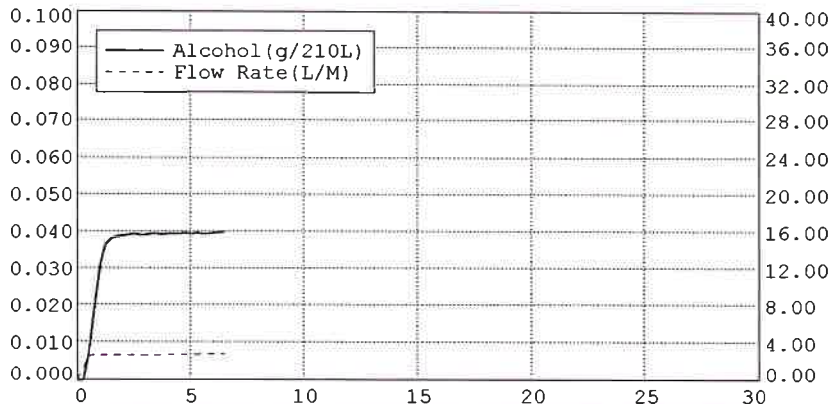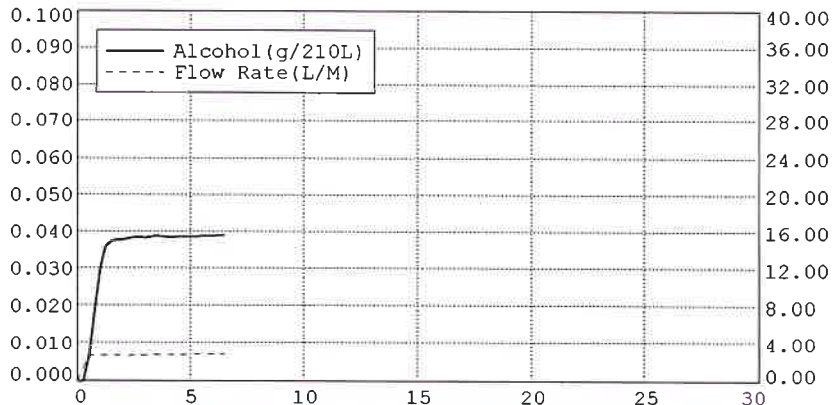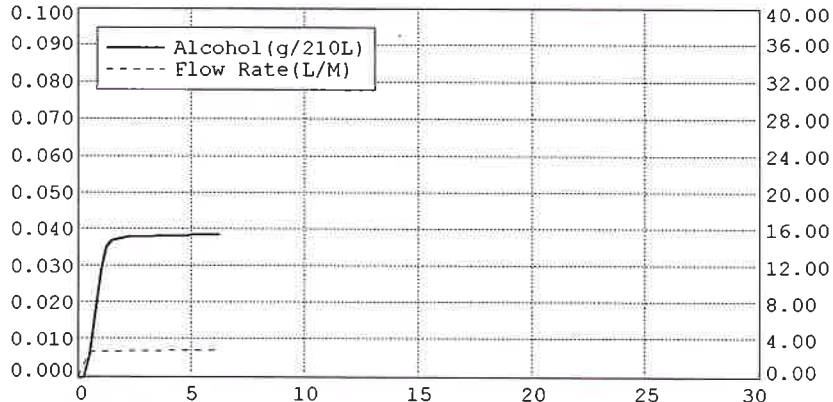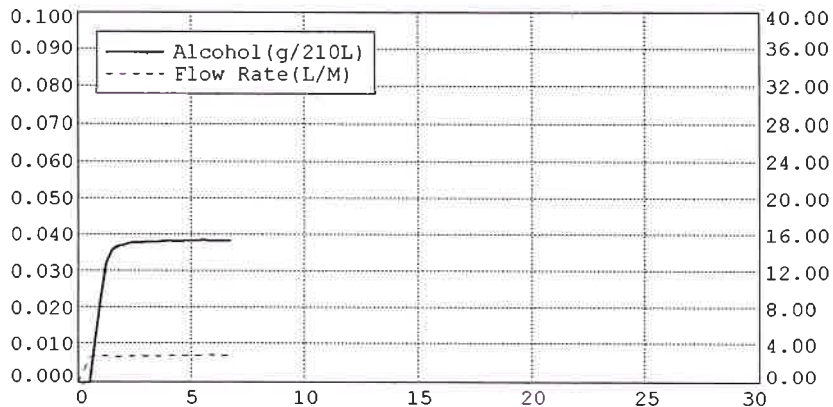

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100422






Date: 04/29/2025
Time: 09:10:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 361 psi

BLANK TEST	0.000	09:12
INTERNAL STANDARD	VERIFIED	09:12
EXTERNAL STANDARD	0.078	09:12
BLANK TEST	0.000	09:13
EXTERNAL STANDARD	0.078	09:13
BLANK TEST	0.000	09:14
EXTERNAL STANDARD	0.078	09:14
BLANK TEST	0.000	09:15
EXTERNAL STANDARD	0.079	09:15
BLANK TEST	0.000	09:16
EXTERNAL STANDARD	0.079	09:17
BLANK TEST	0.000	09:18

Average = 0.0784
Std Dev = 0.0005

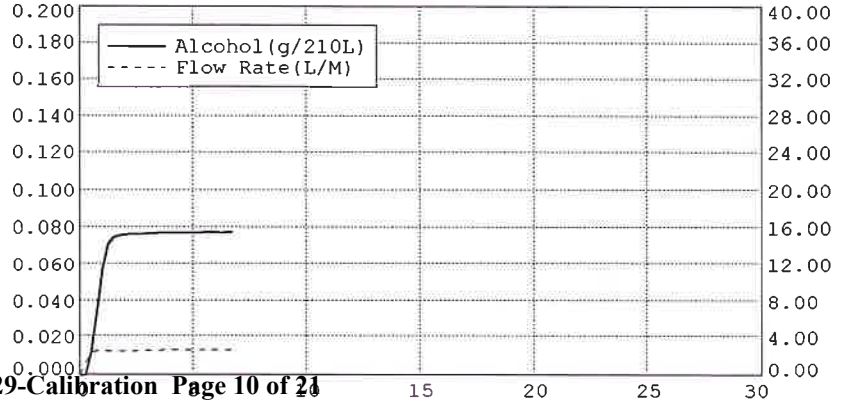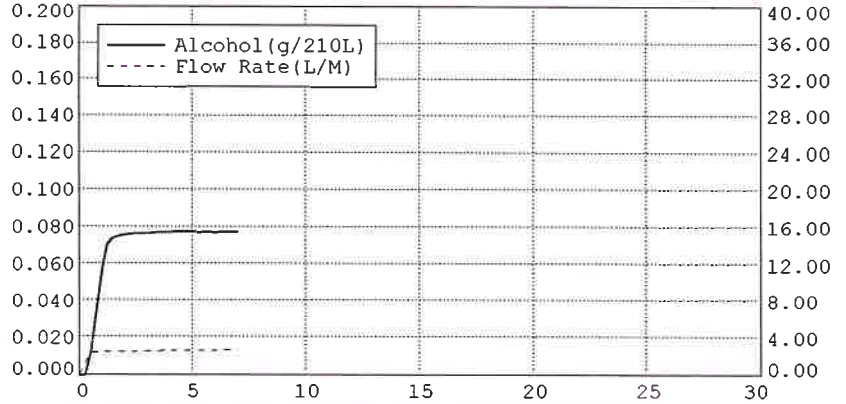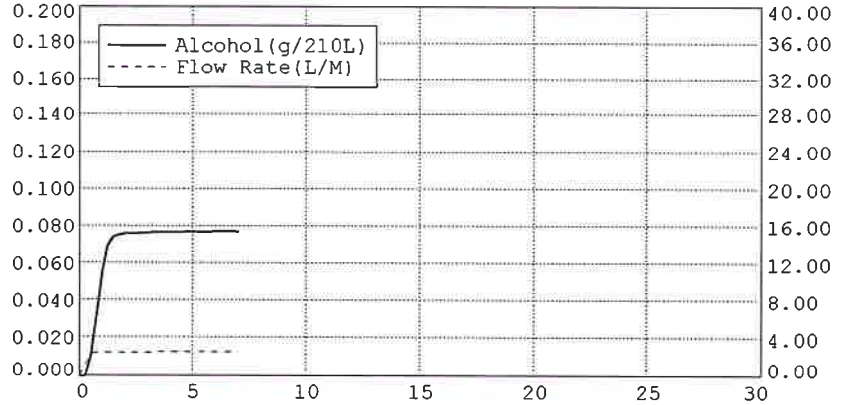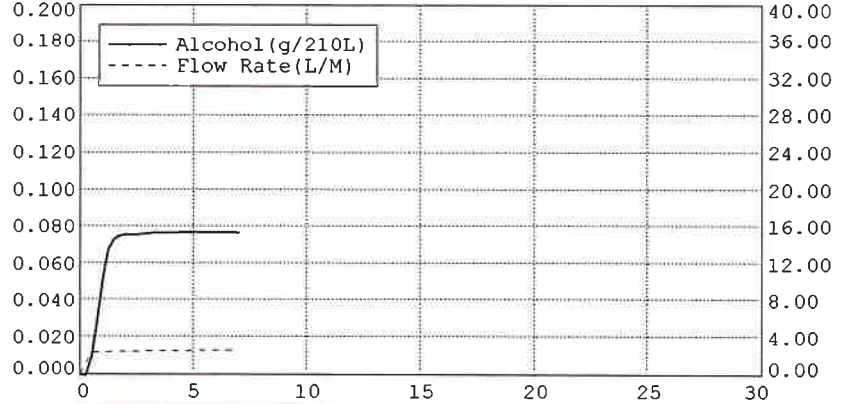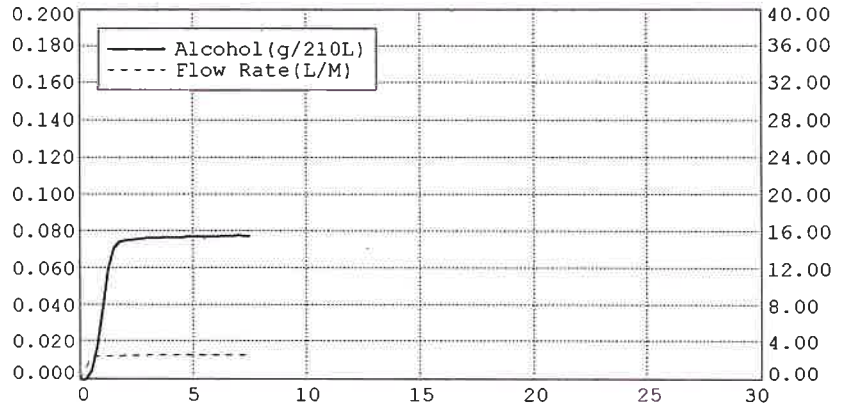

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100422






Date: 04/29/2025
 Time: 09:19:03

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.44: 0.098
 LOT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 1089 psi

BLANK TEST	0.000	09:20
INTERNAL STANDARD	VERIFIED	09:20
EXTERNAL STANDARD	0.100	09:20
BLANK TEST	0.000	09:21
EXTERNAL STANDARD	0.099	09:22
BLANK TEST	0.000	09:22
EXTERNAL STANDARD	0.099	09:23
BLANK TEST	0.000	09:24
EXTERNAL STANDARD	0.099	09:24
BLANK TEST	0.000	09:25
EXTERNAL STANDARD	0.100	09:25
BLANK TEST	0.000	09:26

Average = 0.0994
 Std Dev = 0.0005

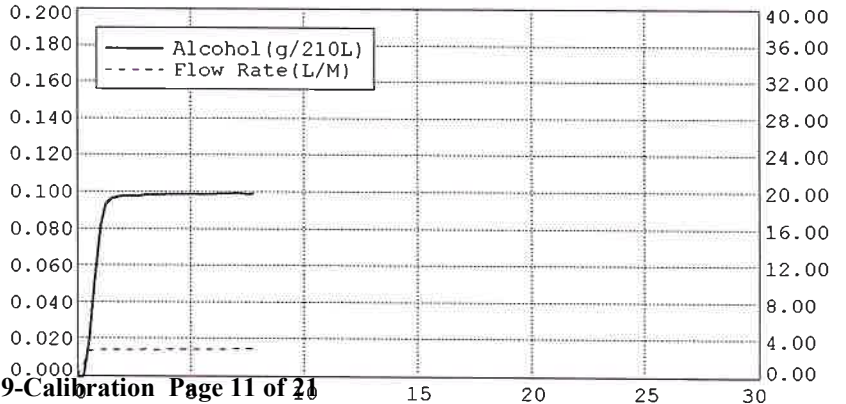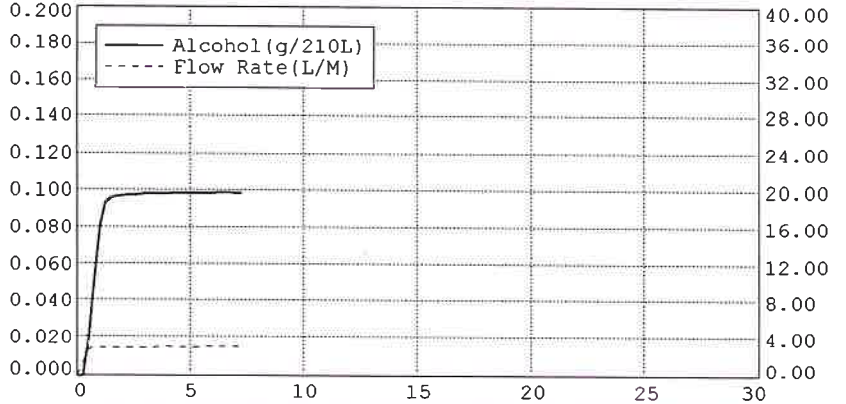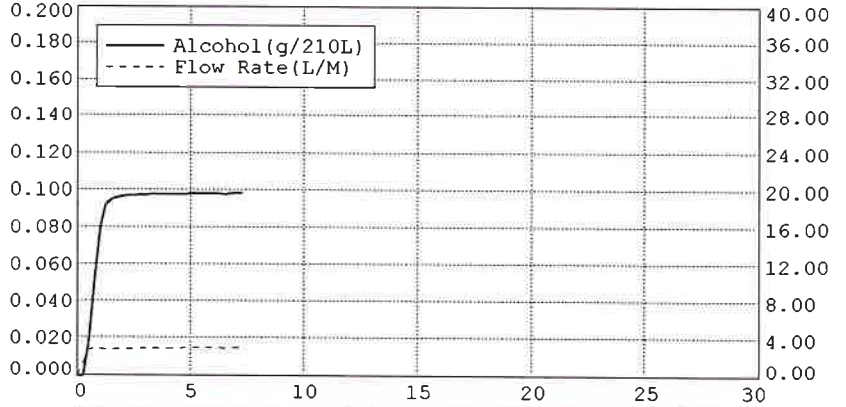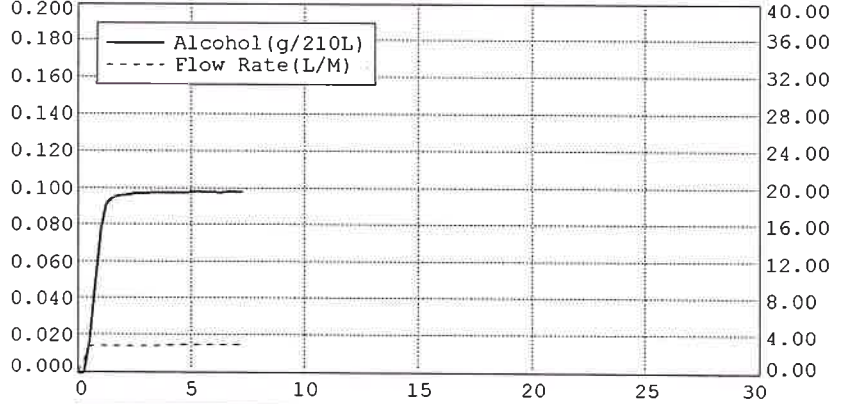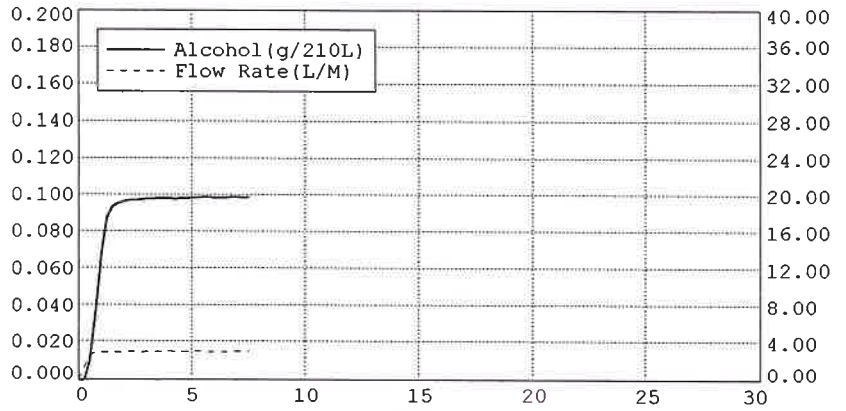

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100422






Date: 04/29/2025
 Time: 09:27:00

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.44: 0.148
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 362 psi

BLANK TEST	0.000	09:28
INTERNAL STANDARD	VERIFIED	09:28
EXTERNAL STANDARD	0.147	09:28
BLANK TEST	0.000	09:29
EXTERNAL STANDARD	0.146	09:29
BLANK TEST	0.000	09:30
EXTERNAL STANDARD	0.146	09:30
BLANK TEST	0.000	09:31
EXTERNAL STANDARD	0.145	09:32
BLANK TEST	0.000	09:33
EXTERNAL STANDARD	0.146	09:33
BLANK TEST	0.000	09:34

Average = 0.1460
 Std Dev = 0.0007

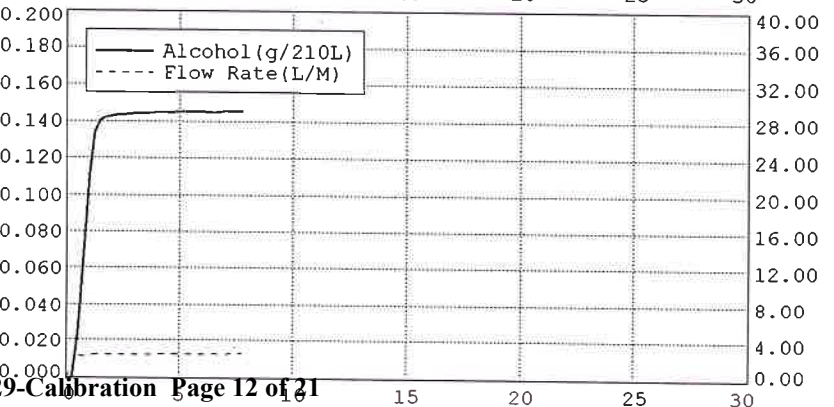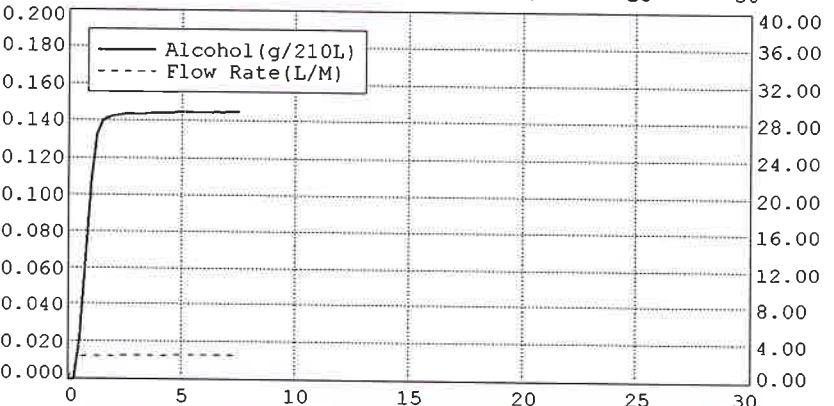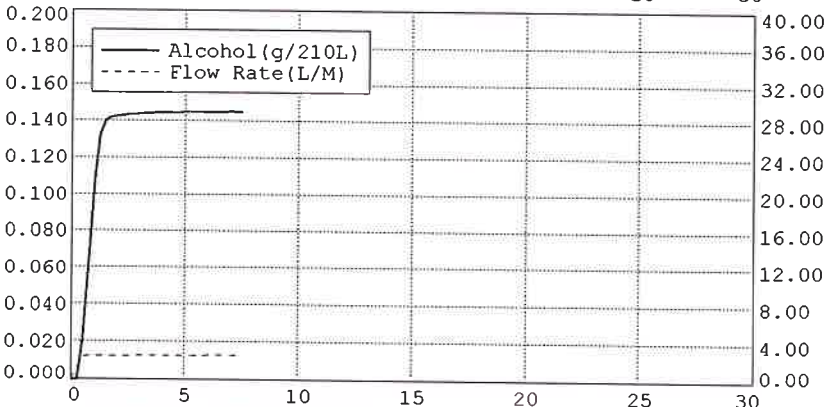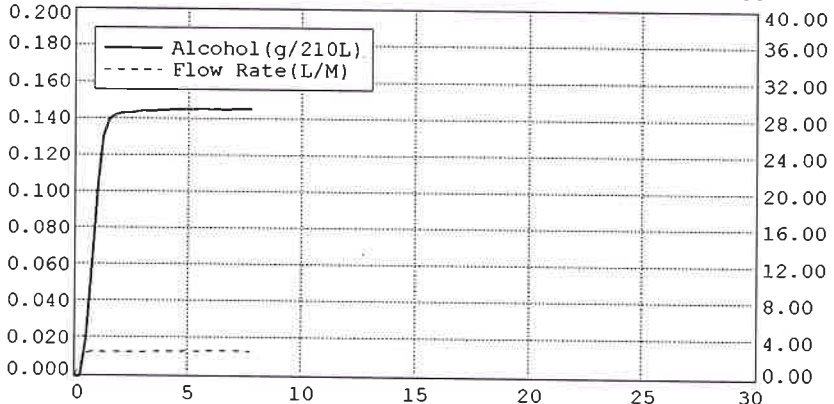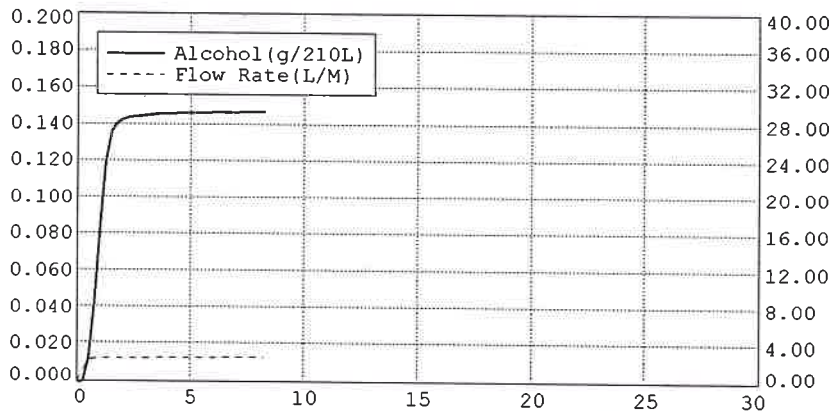

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100422






Date: 04/29/2025
 Time: 09:34:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.44: 0.295
 LOT #: AG427706
 EXPIRATION: 10/03/2026
 TANK PRESSURE: 407 psi

BLANK TEST	0.000	09:36
INTERNAL STANDARD	VERIFIED	09:36
EXTERNAL STANDARD	0.295	09:36
BLANK TEST	0.000	09:37
EXTERNAL STANDARD	0.294	09:37
BLANK TEST	0.000	09:38
EXTERNAL STANDARD	0.295	09:38
BLANK TEST	0.000	09:39
EXTERNAL STANDARD	0.296	09:40
BLANK TEST	0.000	09:41
EXTERNAL STANDARD	0.295	09:41
BLANK TEST	0.000	09:42

Average = 0.2950
 Std Dev = 0.0007

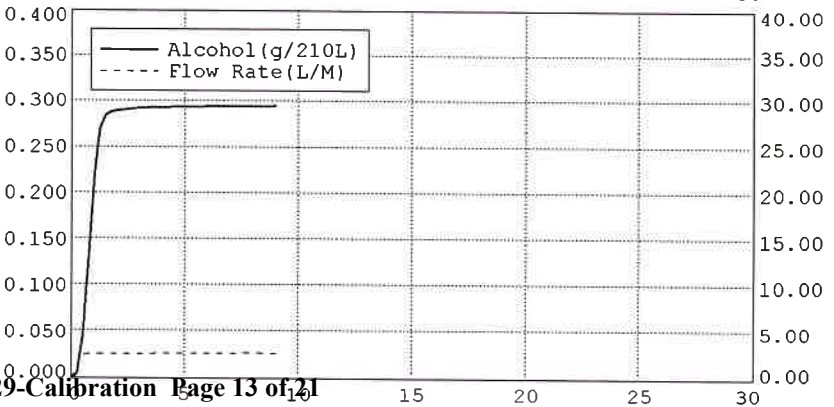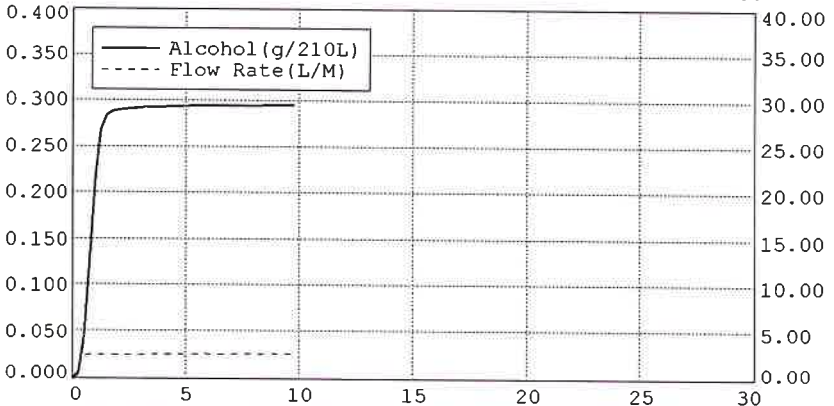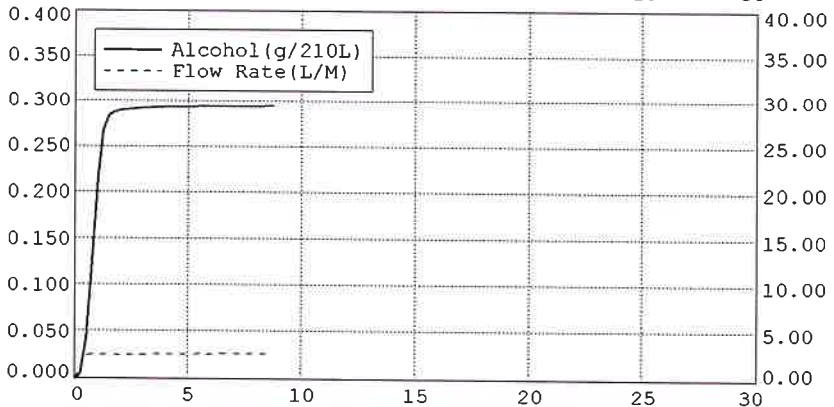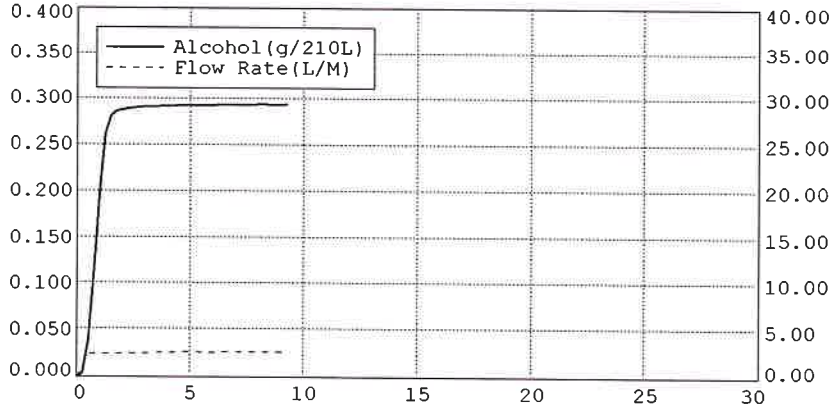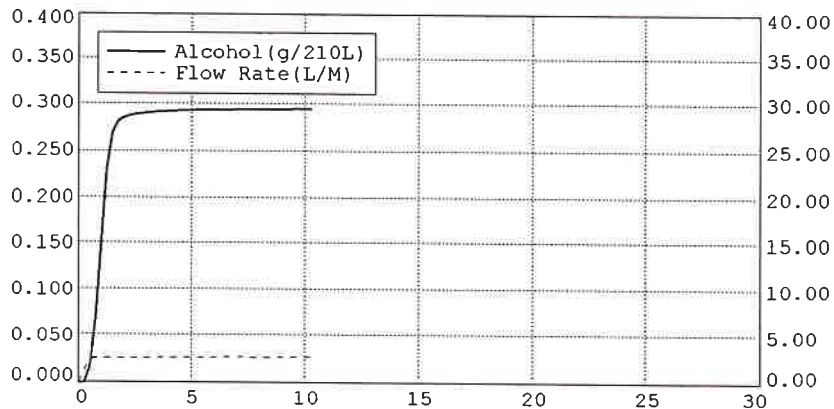

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 09:52:05

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 09:56
BLANK TEST 0.000 09:56
INTERNAL STANDARD VERIFIED 09:56
EXTERNAL STANDARD 0.079 09:56
BLANK TEST 0.000 09:57
SUBJECT SAMPLE INCOMPLETE 09:59

KS

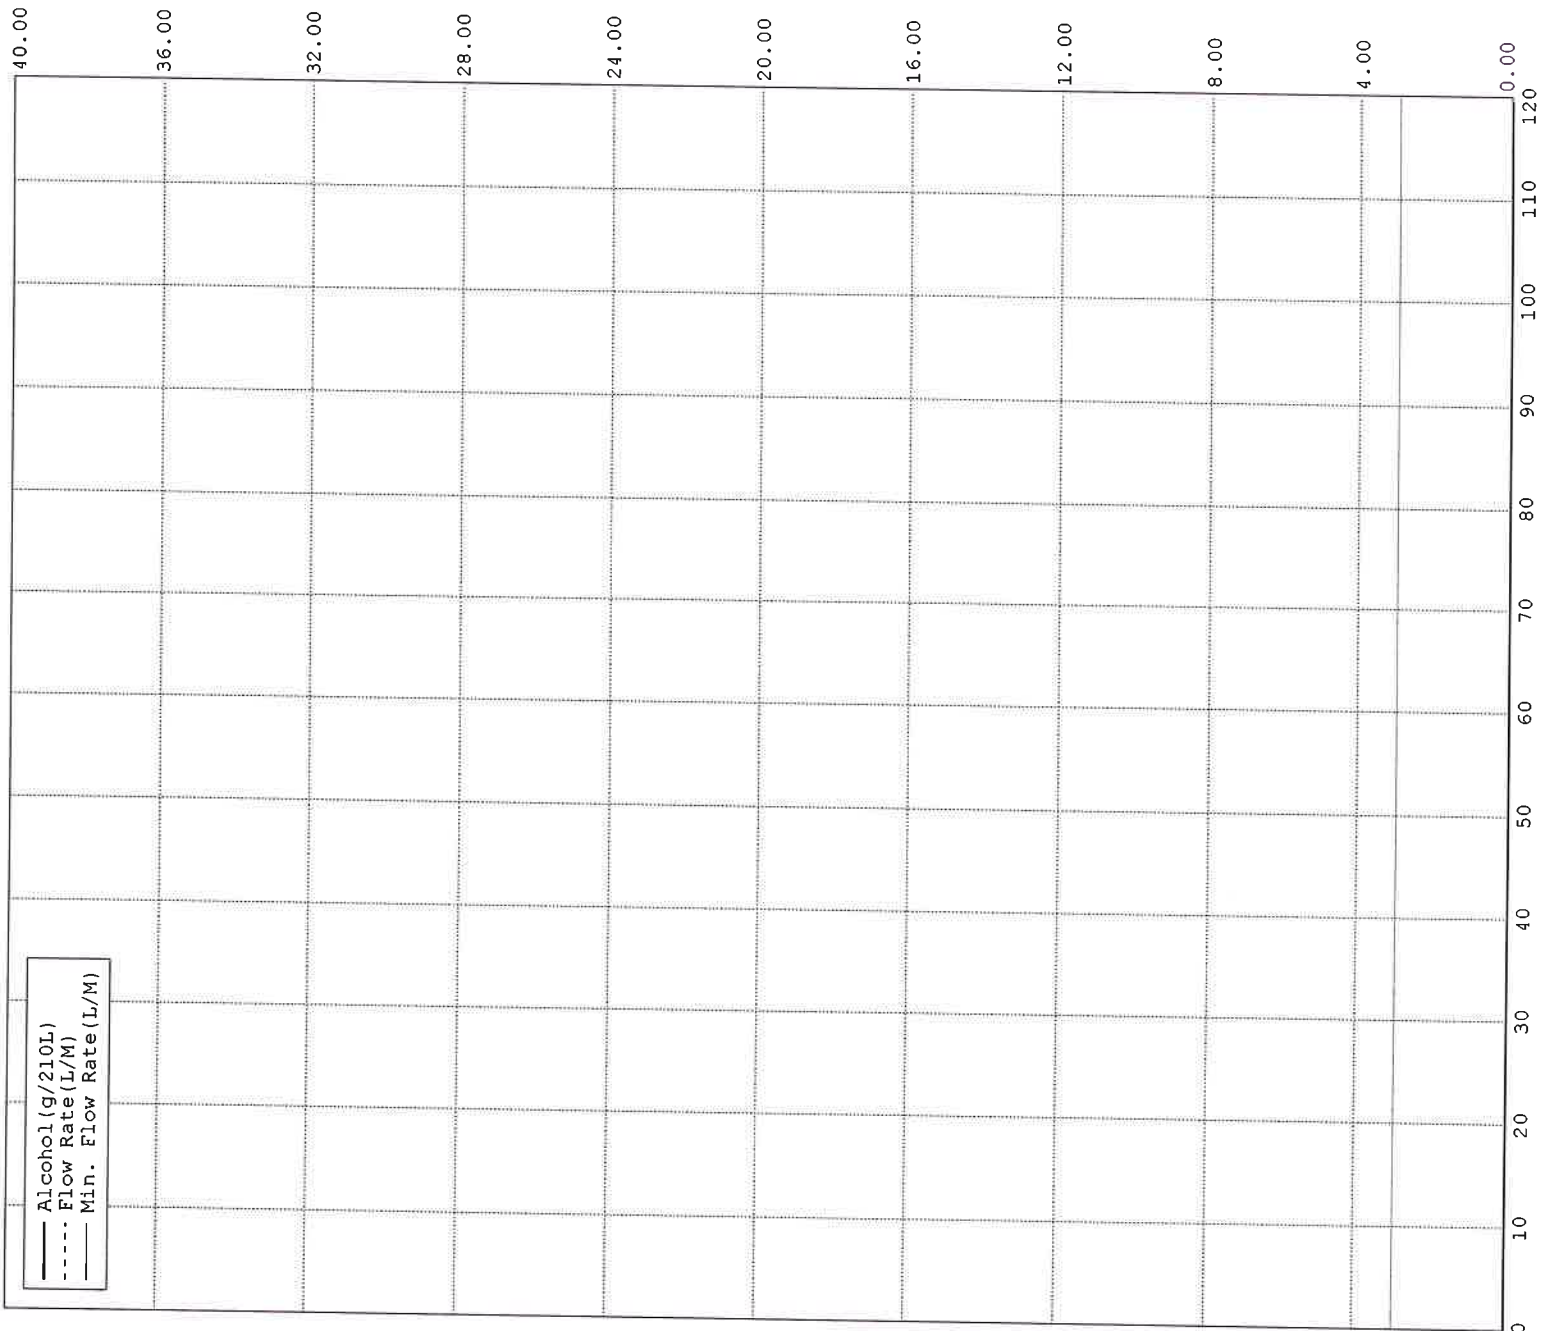

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 10:01:33

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 10:02
BLANK TEST 0.000 10:02
INTERNAL STANDARD VERIFIED 10:02
EXTERNAL STANDARD 0.078 10:03
BLANK TEST 0.000 10:04
SUBJECT SAMPLE XXX 10:04

Maximum Attempts Exceeded

KS

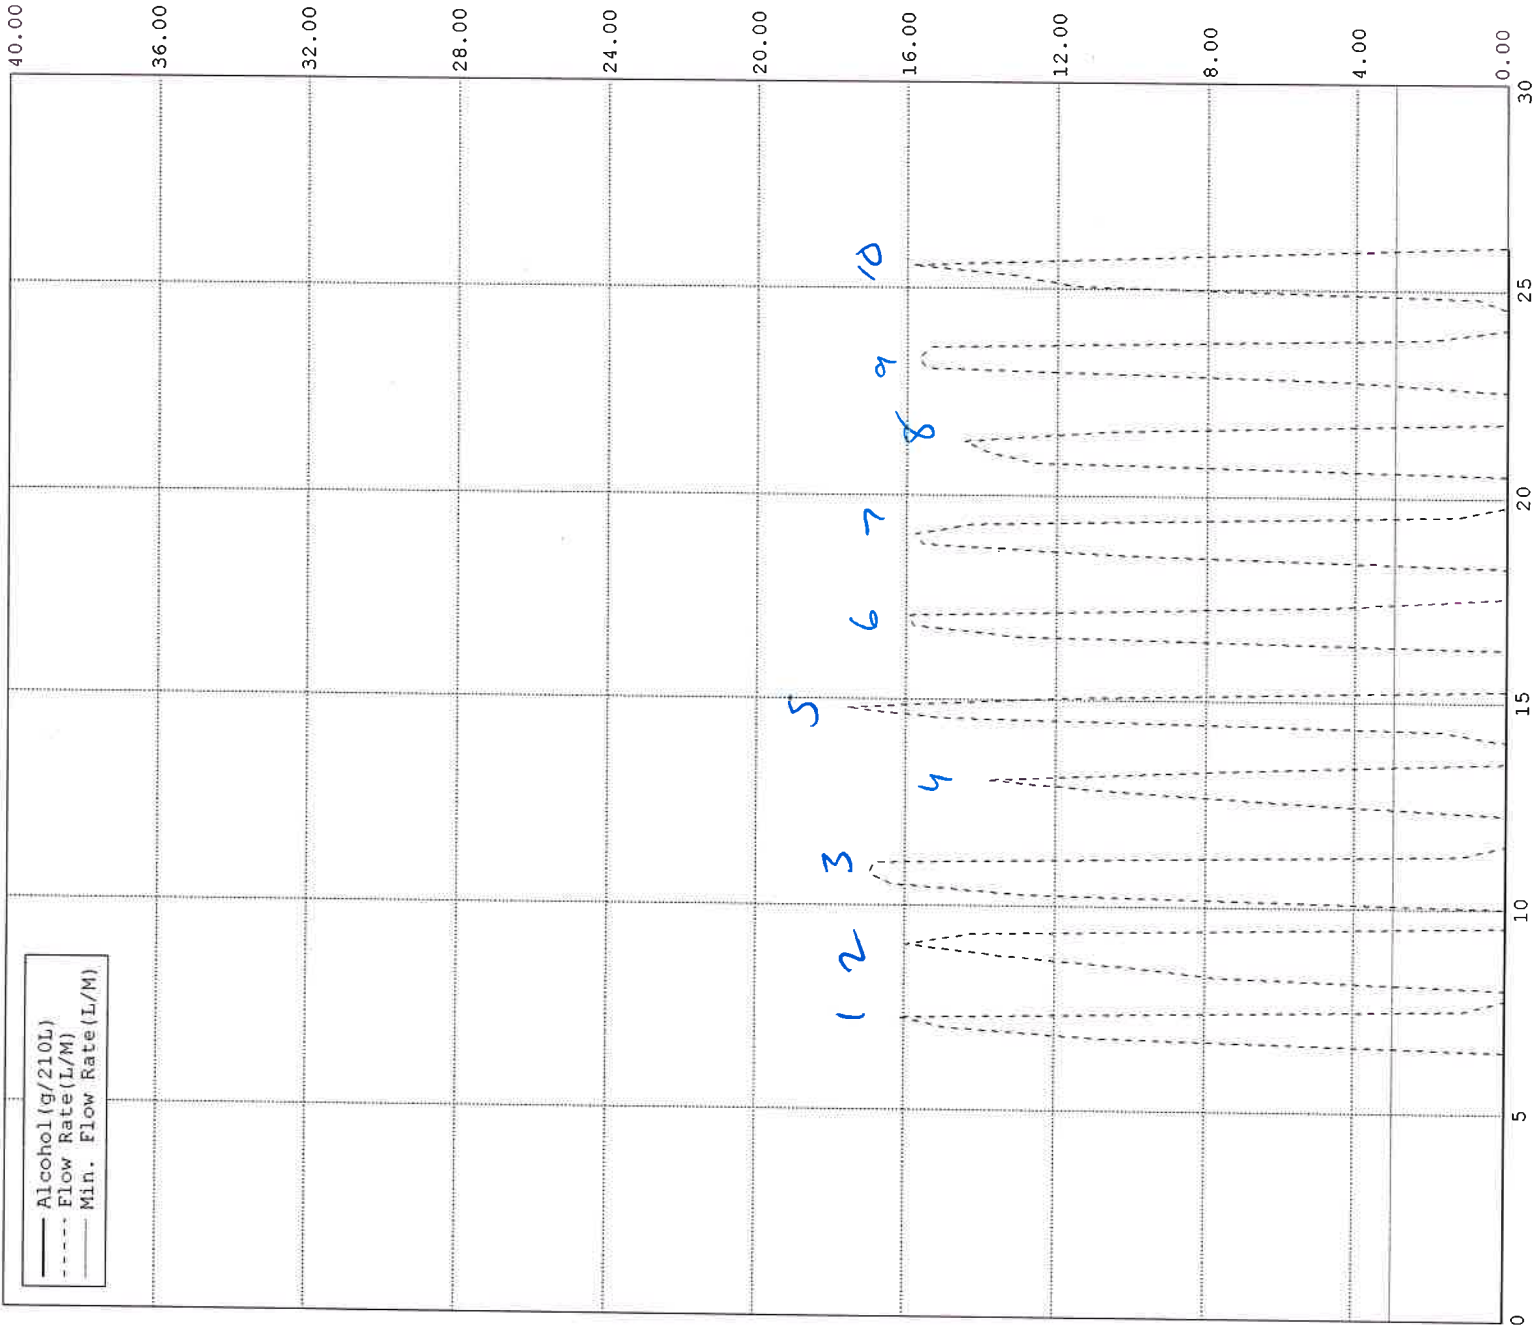

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 10:06:11

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAJJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:

~~MAXIMUM ATTEMPTS EXCEEDED~~

CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:07
BLANK TEST	0.000	10:07
INTERNAL STANDARD	VERIFIED	10:07
EXTERNAL STANDARD	0.078	10:07
BLANK TEST	0.000	10:08
SUBJECT SAMPLE	INVALID	10:09

*Invalid
KS 4/29/25*

*KS - invalid
4/29/25*

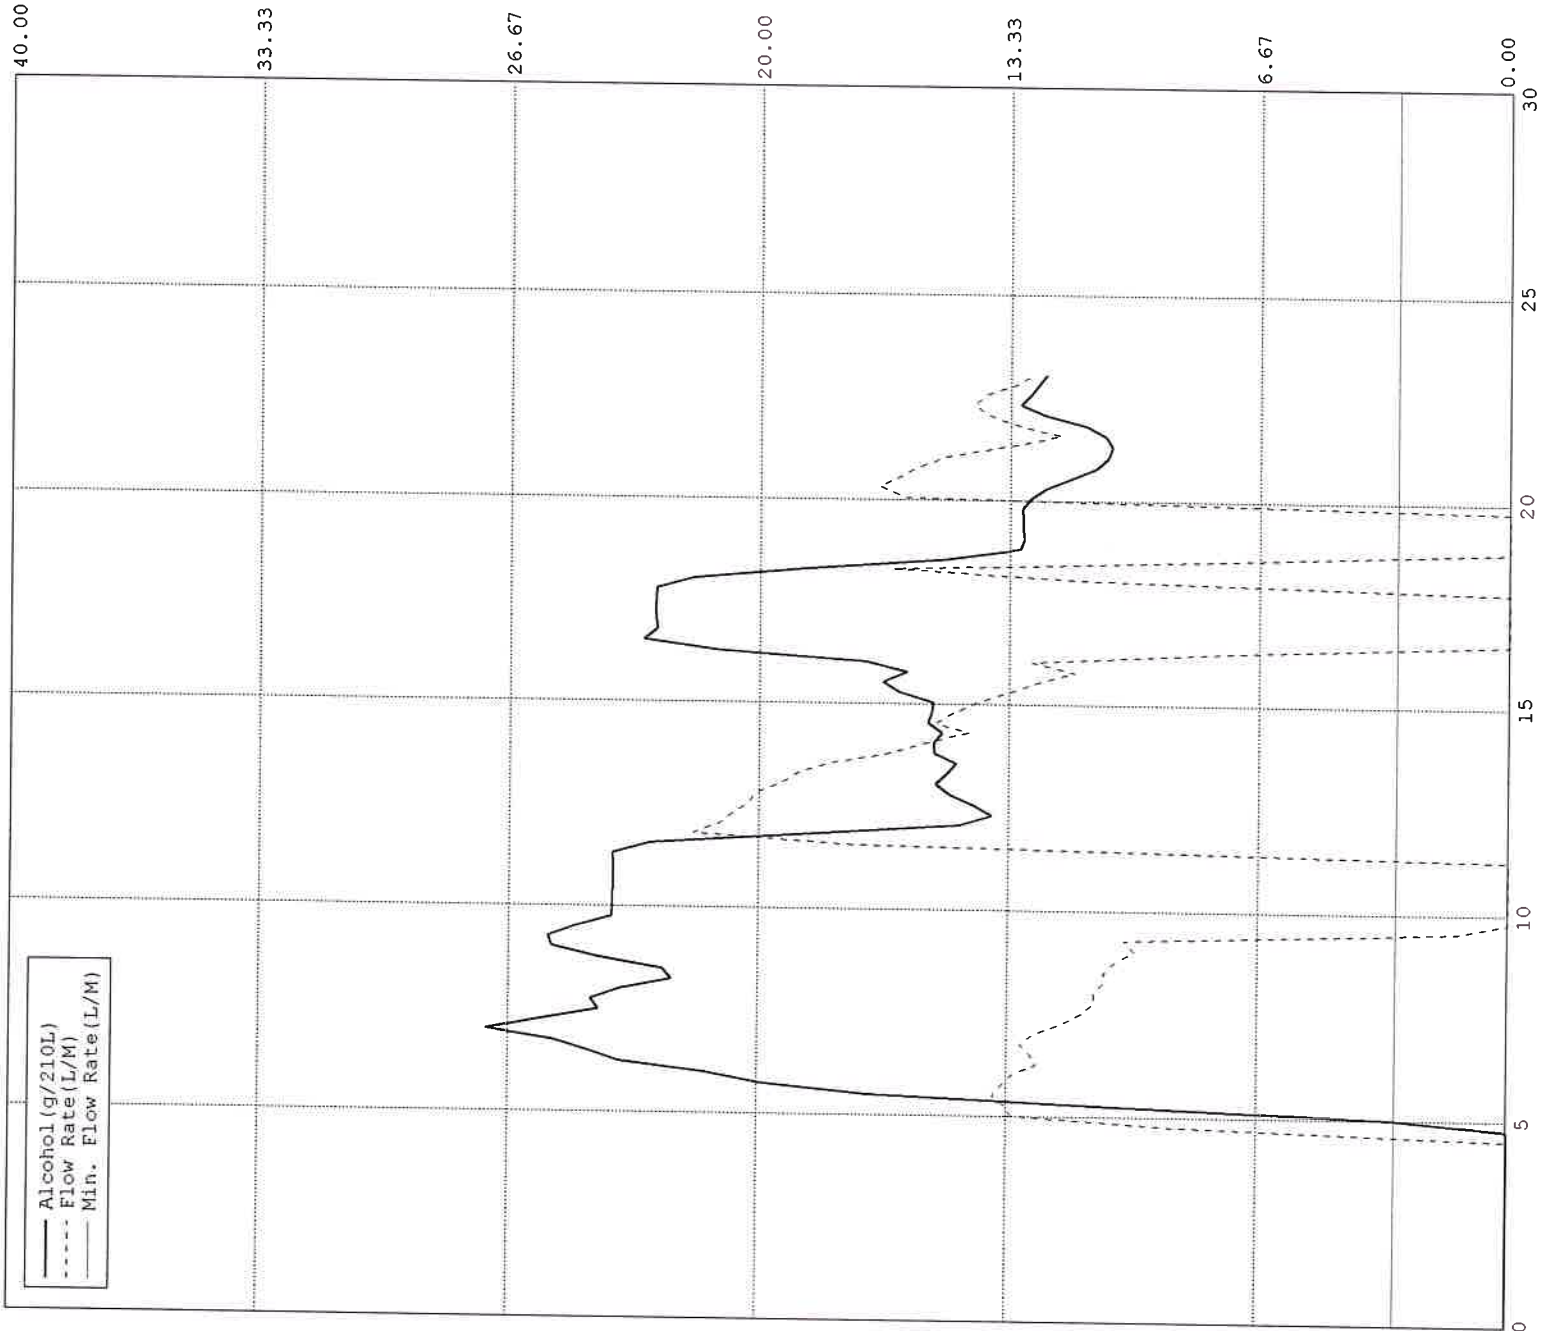

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 10:10:46

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
RFI

CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.43: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 10:14
BLANK TEST 0.000 10:14
INTERNAL STANDARD VERIFIED 10:14
EXTERNAL STANDARD 0.078 10:14
BLANK TEST 0.000 10:15

RFI DETECTED

KS

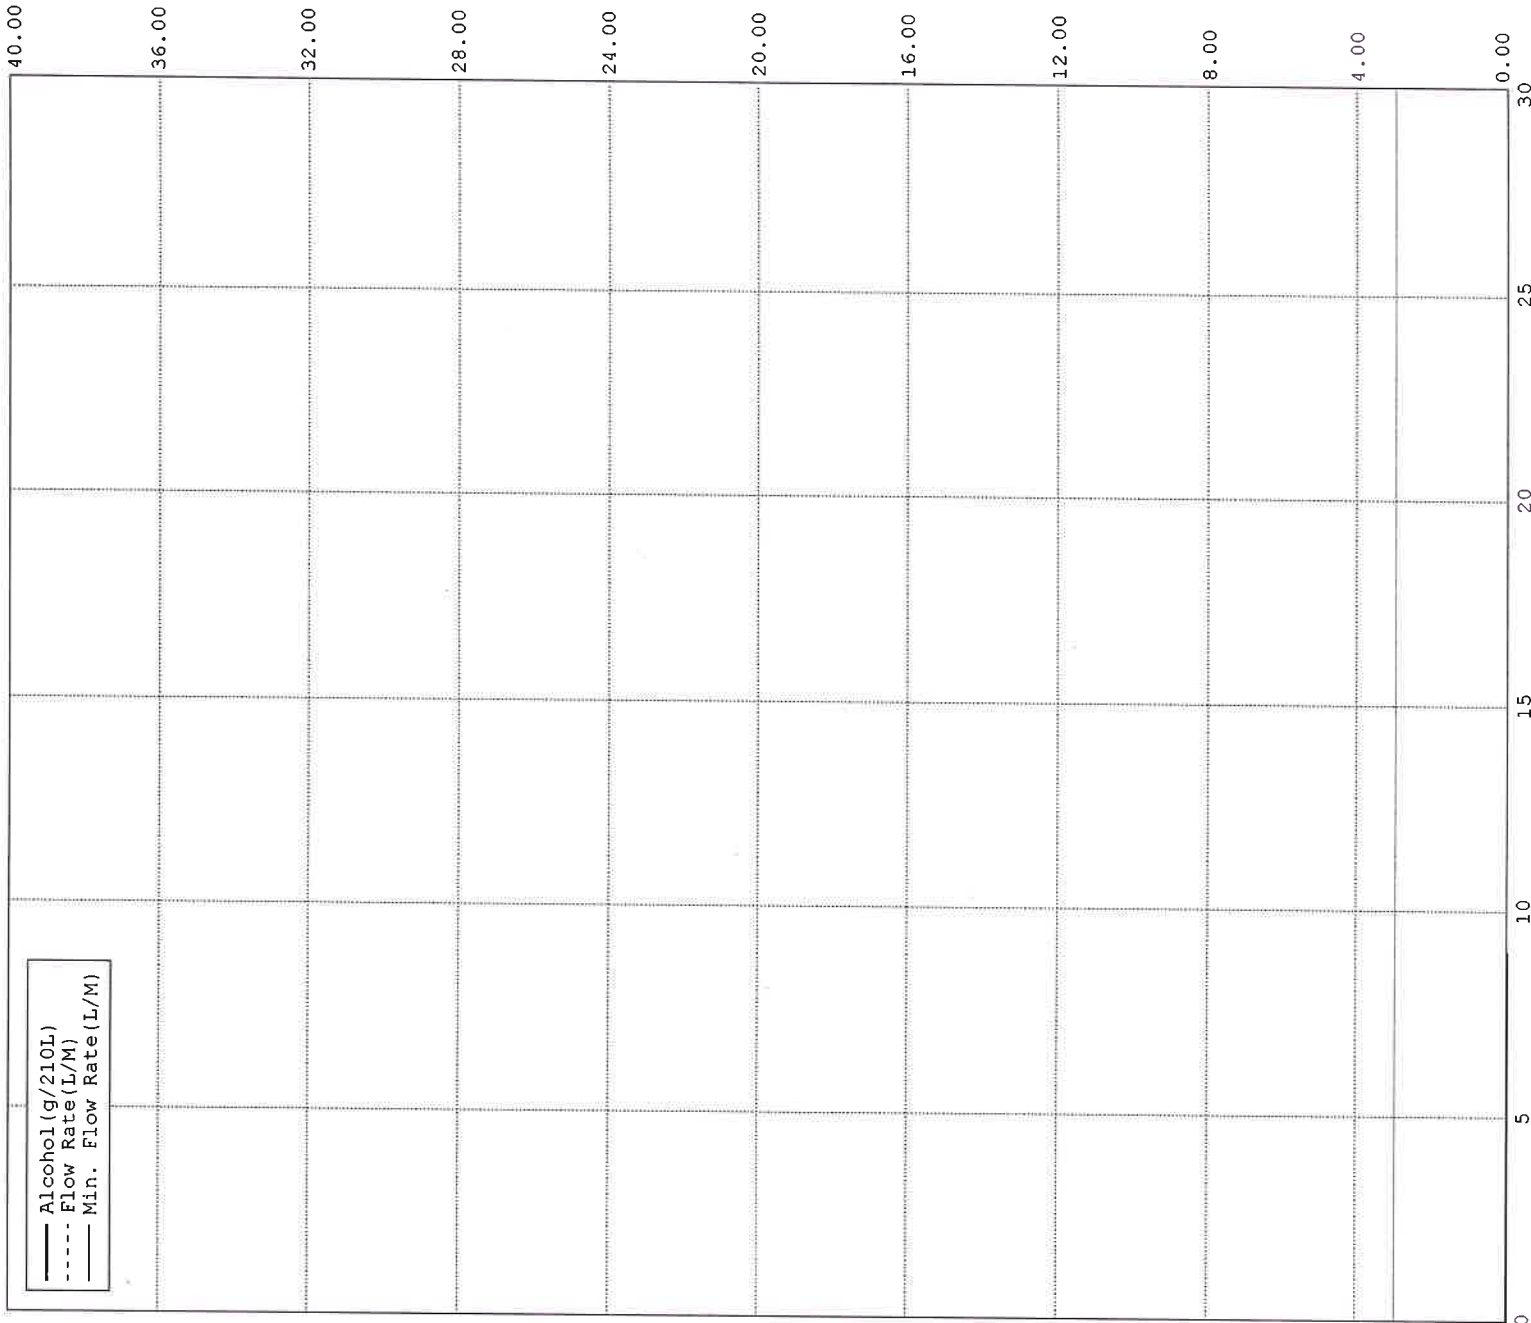

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 11:10:46

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
ACETONE

CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:11
BLANK TEST 0.000 11:11
INTERNAL STANDARD VERIFIED 11:12
Xq = 0.110 (0.64%) 0.079 11:12
EXTERNAL STANDARD X[1] = 0.0788 (-0.0002) (0.0016) 0.000 11:13
BLANK TEST XXX 11:13
SUBJECT SAMPLE X[1] = 0.1094 (-0.0188) (0.0006)

Interference Detected

Filter 2ave: -0.0009
Filter 3ave: 0.0018
KS 4/29/25

KS



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 11:05:46

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
IPA

CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:06
BLANK TEST 0.000 11:06
INTERNAL STANDARD VERIFIED 11:07
Xq = 0.109 (0.56%)
EXTERNAL STANDARD 0.078 11:07
X[1] = 0.0776 (-0.0024) (0.0028)
BLANK TEST 0.000 11:08
SUBJECT SAMPLE XXX 11:08
X[1] = 0.1195 (-0.0315) (0.0017)

Interference Detected

100422-2025-04-29 Calibration # 19 of 21

KS

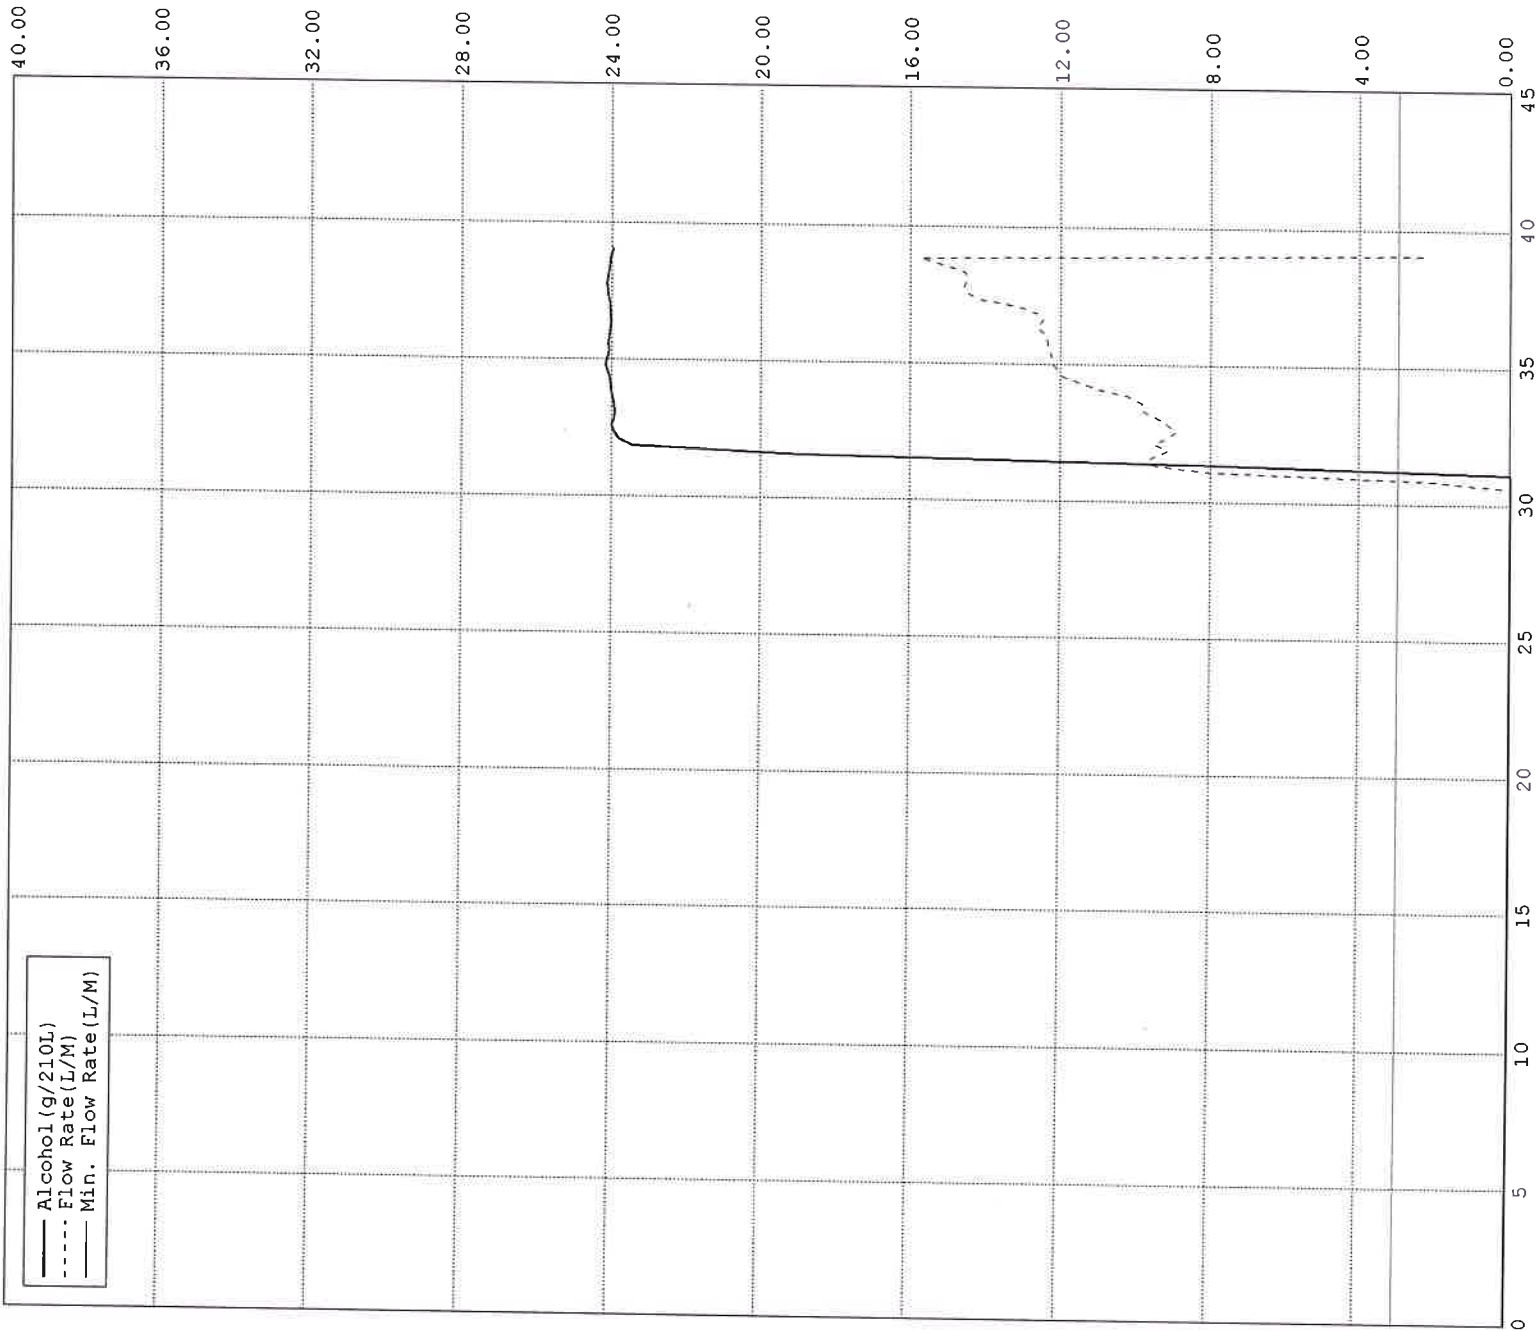

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 11:15:25

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.090
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:16
BLANK TEST 0.000 11:16
INTERNAL STANDARD VERIFIED 11:16
Xq = 0.110 (0.72%)
EXTERNAL STANDARD 0.078 11:16
X[1] = 0.0785 (-0.0014) (0.0015)
BLANK TEST 0.000 11:17
SUBJECT SAMPLE (Vol=1.60L) 0.093 11:18
X[1] = 0.0939 (-0.0019) (0.0007)
BLANK TEST 0.000 11:19
EXTERNAL STANDARD 0.078 11:19
X[1] = 0.0784 (0.0006) (0.0012)
BLANK TEST 0.000 11:20

KS

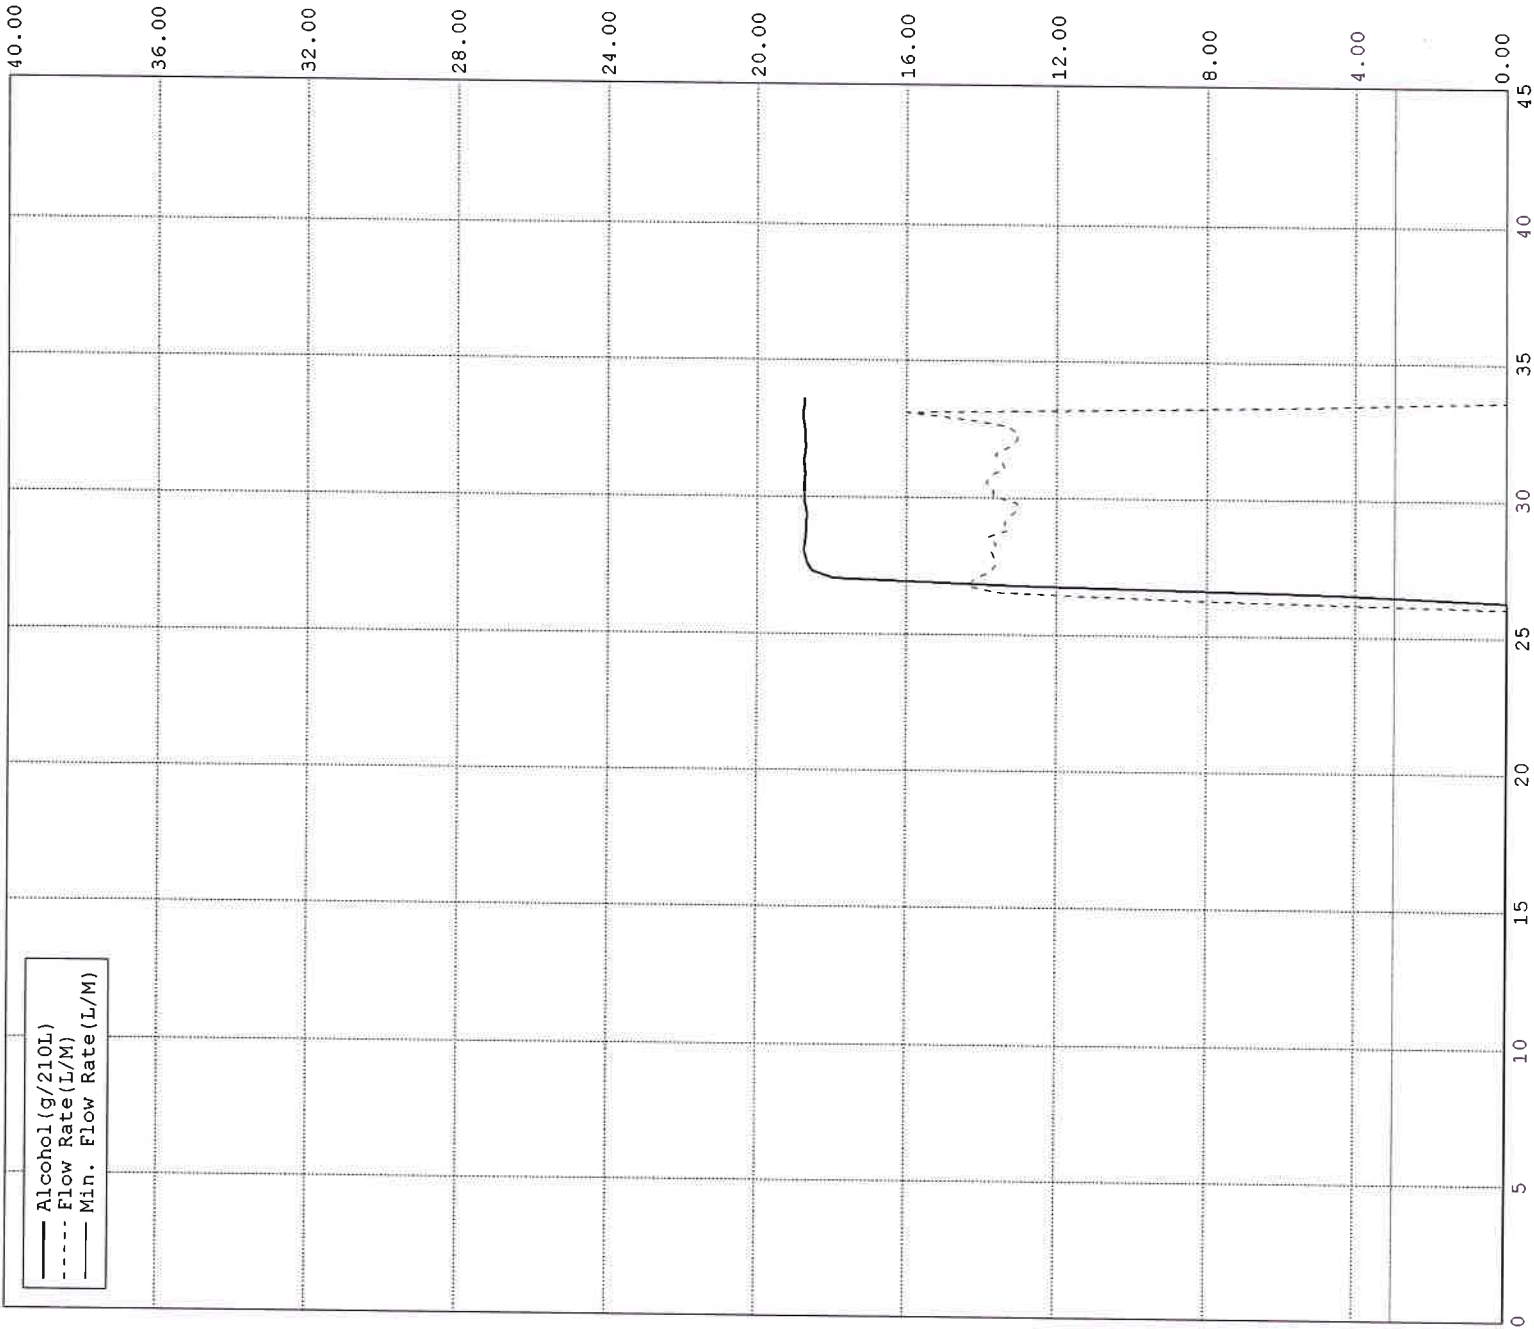

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100422

Date: 04/29/2025
Time: 11:37:56

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.43: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:39
BLANK TEST 0.000 11:39
INTERNAL STANDARD VERIFIED 11:39
EXTERNAL STANDARD 0.078 11:39
BLANK TEST 0.000 11:40
SUBJECT SAMPLE (Vol=1.84L) 0.000 11:40
BLANK TEST 0.000 11:41
EXTERNAL STANDARD 0.079 11:41
BLANK TEST 0.000 11:42

KS

